



This is a self-archived – parallel-published version of an original article. This version may differ from the original in pagination and typographic details. When using please cite the original.

AUTHOR Niela-Vilen, Hannakaisa;
Azimi, Iman; Suorsa, Kristin; Sarhaddi,
Fatemeh; Stenholm, Sari; Liljeberg,

Pasi; Rahmani, Amir M.; Axelin, Anna

TITLE Comparison of Oura Smart Ring
Against ActiGraph Accelerometer for
Measurement of Physical Activity and
Sedentary Time in a Free-Living
Context

YEAR 2022

DOI 10.1097/CIN.0000000000000885

VERSION Final Draft

CITATION Niela-Vilen, Hannakaisa
PhD; Azimi, Iman PhD; Suorsa,
Kristin PhD; Sarhaddi, Fatemeh MSc;
Stenholm, Sari PhD; Liljeberg, Pasi
PhD; Rahmani, Amir M. PhD; Axelin,
Anna PhD. Comparison of Oura
Smart Ring Against ActiGraph
Accelerometer for Measurement of
Physical Activity and Sedentary Time in
a Free-Living Context. CIN:
Computers, Informatics, Nursing:
February 28, 2022 - Volume - Issue -
doi: 10.1097/CIN.0000000000000885

Comparison of Oura smart ring against ActiGraph accelerometer for measurement of physical activity and sedentary time in a free-living context

Abstract

Smart rings, such as the Oura ring, might have potential in health monitoring. To be able to identify optimal devices for healthcare settings, validity studies are needed. The aim of this study was to compare the Oura smart ring estimates of steps and sedentary time with data from the ActiGraph accelerometer in a free-living context. A cross-sectional observational study design was used. A convenience sample of healthy adults ($n = 42$) participated in the study and wore an Oura smart ring and an ActiGraph accelerometer on the non-dominant hand continuously for one week. The participants completed a background questionnaire and filled out a daily log about their sleeping times and times when they did not wear the devices. The median age of the participants ($n = 42$) was 32 years (range 18-46 years). In total, 191 (61% of the potential) days were compared. The Oura ring overestimated the step counts compared with the ActiGraph. The mean difference was 1416 steps (95% CI 739 to 2093 steps). Daily sedentary time was also overestimated by the ring; the mean difference was 17 minutes (95% CI -2 to 37 min). The use of the ring in nursing interventions needs to be considered.

Key words: accelerometer; physical activity; sedentary; smart ring; validation

INTRODUCTION

For healthcare professionals, it is often important to map holistically all the aspects associated with the patient's well-being. Physical activity is one of the essential elements related to a healthy lifestyle; an adequate level of physical activity promotes, for example, the ability to function and weight control. Furthermore, physical activity reduces the risk for certain diseases. Inadequate physical activity, however, is a global phenomenon. ¹ Only some adults, as well as children and adolescents, achieve the internationally recommended levels of physical activity. Low levels of physical activity and excessive sedentary behaviour, defined as sitting, reclining, or lying down while awake, are associated with many health-related risks such as diabetes and cardiovascular diseases. ^{1,2} It is also typical for individuals to overestimate the volume and intensity of their physical activity when reported subjectively.

^{3,4} Furthermore, possible changes in health behaviours require time. Therefore, objective and long-term measurement of physical activity is needed. Commercially available small and lightweight wearable activity trackers might be useful in healthcare settings as well as in nursing interventions. It is also suggested that nurses could use activity trackers as an opportunity to encourage people to engage in physical activity. ⁵

Commercially available wearable activity trackers have become very popular for monitoring physical activity. Following many wrist-worn smart bands and smartwatches, a finger-worn smart ring has come to the market. Smart rings such as the Oura ring (<https://ouraring.com/>) provide a different option to more traditional smartwatches and smart bands. Rings might attract users as they are more like pieces of jewellery instead of watches. Wearable trackers might have the potential to facilitate physical activity in individuals; however, multifaceted interventions seem to have greater effect compared with a wearable activity tracker only. ^{6,7} Previously, wrist-worn activity trackers have shown value for patients with chronic diseases,

such as cancer or diabetes, or specific populations such as children or older adults. ⁸Users' feedback has been mostly positive; users have found activity trackers appealing and useful for increasing their levels of physical activity. ⁹

In addition to health care settings, wearable activity trackers are also used in measuring for research purposes, as they are comfortable and easy to use in participants' daily life and provide real-time feedback as well as enable continuous assessment of physical activity for long periods of time. ^{6, 8, 10-11} The accuracy of wearable trackers is essential for individuals, nurses and other healthcare professionals, as well as researchers; therefore, establishing the validity and accuracy of activity trackers is important. ¹² The performance of activity trackers, especially in a free-living context, should be examined further to identify optimal devices, for example, for research purposes. ¹³ New devices are released every year, and technological advances in those provide new possibilities to researchers. ¹² The majority of previous validity studies have been conducted with wrist-worn trackers.

Studies about the Oura smart ring have provided promising results about its validity concerning sleep in laboratory conditions against polysomnography both in adults ¹⁴⁻¹⁵ and in adolescents ¹⁶, as well as in a free-living context against wrist-worn actigraphy in a healthy adult population. ¹⁷⁻¹⁸ It has been stated that sleep staging in the Oura ring needs improvement. ¹⁶ Regarding sleep quality, the correlations between the Oura ring and other devices measuring sleep were weak in a pilot study aiming to monitor sleep in the natural environment. It is, however, notable that no golden standard measure was used. ¹⁹ Nocturnal heart rate and heart rate variability of the Oura ring has been validated against ECG with home-based monitoring. Very high agreement was observed between the ring and ECG measurements. ²⁰ Furthermore, the Oura ring has shown potential in monitoring the menstrual cycle based on nocturnal skin temperature. ²¹ The Oura ring has also been tested in detecting

COVID-19²² and predicting symptoms of depression and anxiety.²³ Aside from a preprint study, which was not peer reviewed, there are no previous publications about the validity of the physical activity or sedentary time measures of the Oura ring. The preprint by Henriksen et al.²⁴ showed that the step count was overestimated by the Oura smart ring compared with the ActiGraph placed on the hip.

The aim of this study was to compare the Oura smart ring estimates of steps and sedentary time with data from the ActiGraph accelerometer with healthy adults in a free-living context.

METHODS

Design and setting

A prospective observational study design was performed in southern Finland during July-August 2019. Reporting the study adheres to the STROBE reporting guidelines.

Recruitment and participants

A convenience sample of healthy adults between 18 and 55 years old was recruited for the study. Potential participants were excluded if they had 1) a diagnosed heart disease, 2) restrictions regarding physical activity, 3) the symptoms of illness at the time of recruitment, or 4) any restrictions of using the devices at work.

The research assistants scheduled a meeting with each interested and eligible participant. The purpose of the study was explained, and written informed consent was obtained. The participants were asked to wear an Oura smart ring and an ActiGraph accelerometer (reference device) continuously for one week. The Oura smart ring was placed on a finger of

the non-dominant hand and the ActiGraph on the wrist of the non-dominant hand; thus, both devices were worn on the same hand.

Altogether, 46 participants (23 females and 23 males) were enrolled in the study. One participant was excluded from the analyses due to not wearing the ActiGraph, and three participants were excluded because they did not have enough data for the analyses. Thus, the final sample size was 42.

Measures

The Oura smart ring (Ōura Health Ltd., Finland) is a commercial tracker device for monitoring activity, sleep, heart rate, and heart rate variability. The Oura ring includes one built-in photoplethysmography sensor and an inertial measurement unit (IMU). The ring is light (4–6 grams), waterproof, and easy to use. The battery life is six days. The data are automatically sent to the mobile app (compatible with both Android and iOS) and transferred to the cloud server.

The ActiGraph accelerometer (Pensacola, FL, USA) is a non-commercial device for research purposes and was used as a reference measure in this study. The battery life is 25 days. The ActiGraph measurements are based on motion sensors that provide data for numerous activity measures. In this study, a wrist-worn ActiGraph wActiSleep-BT was used as it was considered a valid measure. The ActiGraph accelerometer worn on a non-dominant wrist has been shown to overestimate the daily step count by approximately 10% when compared to video observation in free-living conditions ²⁵.

ActiGraph data were downloaded and converted into 60-second epochs using ActiLife software, version 6.13 (ActiGraph, Pensacola, Florida). Sleep time was defined using the algorithm available in ActiLife ²⁶ and non-wear time by the Choi algorithm ²⁷; both sleep and

non-wear time were excluded from the analyses. Sedentary time was defined using the count cut point value of <1853 vector magnitude counts per minute, which is validated for triaxial accelerometers worn on a non-dominant wrist against a thigh-worn triaxial activPAL accelerometer.²⁸ Step count was calculated using ActiLife's step counting algorithm without the low-frequency extension. The Oura ring provides various well-being and health-related parameters, including sleep duration, step counts, non-wear time, rest duration, and inactive time per day. We used the step counts per day values provided by Oura as a measure of physical activity. The sedentary time was also computed as the time when the user was inactive or resting during the day. Moreover, we calculated the wear time per day by subtracting the sleep time and non-wear time from 24 hours. A valid day was defined as a measurement day with a minimum of 10 hours of waking wear time of both the ActiGraph and Oura.

Data collection

The participants were asked to wear the devices continuously for one week in their normal daily life. Verbal guidance and written instructions about using the devices was provided to all participants. Both devices were waterproof; thus, wearing them during a shower or swimming was possible. However, the participants were asked to remove the devices for the sauna. Participants were blinded to the data; they could not follow their activity, such as step count, as the devices had no display or synchronized software available for the participants. The data regarding physical activity were stored in the devices and downloaded after the data collection week by the researchers.

During the study week, the participants were asked to fill in a daily log to record waking time, bedtime, and the periods when they had possibly removed one or both of the devices.

A short questionnaire was completed during the recruitment meeting. The questionnaire included questions about background characteristics (age, weight, height, marital status, education, working status, and smoking) and a question about the frequency of physical activity.

Ethics

The study protocol received a favourable statement from the Ethics Committee for Human Sciences at the University of Turku (Statement 44/2019). Both verbal and written information was provided to the participants before obtaining the written informed consent. All participants had the right to withdraw from the study at any phase and without any specific reason. Each participant was given a gift card (20 euro) to a grocery store to compensate for their time and effort used for the data collection period.

Data analysis

In total, 289 valid days were recorded by ActiGraph and 264 by the Oura ring. The number of common valid days for both devices was 232. Based on the participants' diaries, 41 days were further excluded from the analyses due to the differences of more than 10 minutes in wake wear time between the devices, resulting in an analytical sample of 191 days.

Hierarchical linear mixed method was used to determine the mean difference between the devices. The Pearson correlation coefficients on pairwise step counts and pairwise sedentary time parameters were obtained to evaluate the linear correlation between the ring and the ActiGraph. We also utilized a linear regression analysis method. In this regard, the data of the devices were fit to linear regression lines. Then, r^2 values were calculated to show the scatter of the data around the lines. In addition, the Bland-Altman analysis was used to investigate the agreement between the devices. Bland-Altman provides the mean bias and $\pm 95\%$

confidence intervals of the step counts and sedentary time collected by the devices. P value lower than 0.05 was considered statistically significant.

RESULTS

Participants

A total of 42 participants participated in the study, and 191 days (mean 4.5 days per participant) were compared. The median age of the participants was 32 years, ranging from 18 to 46 years. Their median BMI was in the normal range; however, the sample also included participants with very low and high BMI (Table 1).

Step counts

The Oura ring significantly overestimated the step counts compared with the ActiGraph, $p < 0.001$ (Table 2). The mean difference between the Oura ring and ActiGraph was 1416 steps (95% CI 739 to 2093 steps) per day. Bland-Altman plots are presented in Figure 1, showing the mean difference between the tested device and the ActiGraph. For the Oura ring, the 95% limits of agreement were from -4432 steps to 7264 steps.

The Pearson correlation test showed high positive linear correlation between the ActiGraph and the Oura ring ($r = 0.83$, $p < 0.001$). Moreover, the step counts of the ring were evaluated using regression analysis. Figure 2 shows the regression lines in red. The r^2 of the ActiGraph and the ring is 0.7, showing that the data are around the regression line. The ideal line (i.e., $y = x$) is also indicated in black to show the best scenario where the step counts of the two sources are identical.

Sedentary time

Daily sedentary time was overestimated by the Oura ring, $p = 0.049$ (Table 2). The mean difference between the Oura ring and ActiGraph was 17 minutes (95% CI -2 to 37 min) per day. Bland-Altman plots are presented in Figure 3. For the Oura ring, the 95% limits of agreement were from -220 minutes to 255 minutes. Pearson correlation test showed moderate linear correlation between the ActiGraph and Oura ring ($r = 0.61$, $p < 0.001$). We also used the regression analysis to evaluate the sedentary time of the ring compared with the ActiGraph. The regression line (in red) and the ideal line (in black) are shown in Figure 4. The r^2 of the ActiGraph and the ring was 0.37.

DISCUSSION

This validation study aimed to compare the Oura ring with the ActiGraph device regarding daily step count and sedentary time in free-living conditions. The results showed significant differences between the estimates of steps and sedentary time from the devices. The Oura ring overestimated both the step counts and sedentary time. The mean difference in step counts was 1416 steps per day and in sedentary time was 17 minutes per day. The different algorithms used in the devices may be one explanation for the detected differences in measured parameters. Although the devices were worn on the same hand, the Oura ring was worn on the finger and the ActiGraph on the wrist; thus, the movements detected may differ, which might explain part of the differences.

The Oura ring overestimated the step count, which was also stated in a previous study comparing a hip-worn ActiGraph with the Oura ring.²⁴ The smaller mean difference detected in this study might be explained by the reference device worn on the same hand as the Oura

ring, not on the hip, as in the study by Henriksen et al.²⁴ Based on these results, the Oura ring cannot unambiguously be recommended to replace the ActiGraph in measuring step counts if the accurate number of steps is the priority. The systematic difference in the step count between the ActiGraph and the Oura ring was reasonable, but 95% limits of agreement were large showing somewhat low validity of the ring in the individual level. The correlation between the devices, however, was high, indicating that the ring has the ability to show group-level differences in step count.

The estimation of sedentary time provided by the ring could be considered accurate, as it was close to the value of the ActiGraph. However, the wrist-worn ActiGraph may underestimate daily sedentary time compared with posture-based estimates of the accelerometer, which is worn on the thigh.²⁸⁻²⁹ In the future, the Oura ring should also be validated against a more accurate posture-based method, such as a thigh-worn accelerometer.

The free-living context seems to provide an additional challenge to the accuracy of activity trackers. Many trackers have shown good validity in treadmill tests but more biased in free-living conditions.¹³ Validation studies with different trackers in normal daily life are needed because choosing a device based on validity in controlled settings does not guarantee validity in a free-living context. Previous papers have found the Oura smart ring to be a valid measure for sleep time¹⁷ and for heart rate³⁰ in a free-living context. Furthermore, the validity of Oura smart ring should be developed as finger-worn activity trackers are light, easy to use, and appealing to users.^{8,31} More validation studies are also needed to support the development of new activity trackers.

The results of this study clearly demonstrate the need to carefully consider the characteristics of an activity tracker when used for research purposes as well as in healthcare settings, for example, in nursing interventions.³² If a tracker is, for example, used as an intervention

instrument to support physical activity, it is essential that the measures provided by the device are valid and reliable. Dozens of low-cost wearable activity trackers are commercially available, with large variations in validity; thus, it is not easy to identify the best possible option.

³³ The choice of a wearable device depends also on which component of physical activity is of interest. ³⁴

The results of this study also have implications for nursing as nurses working in different fields of healthcare are in a key position to support their patients being physically active. ³⁵ Increasing physical activity may be an important part of care, for example, in many chronic conditions. Nurses might benefit from understanding the level of validity of activity trackers because they are increasingly popular but still underutilised in nursing ⁵. It is notable that in clinical healthcare settings, contrary to research purposes, the accuracy of the device cannot be the only criterion when weighing up the alternatives. Most importantly, the patients or clients need to find the device appealing and easy to use in their normal daily life. ³⁴ Further, if the device is able to show the progress in physical activity and, by implication, to support the patient to stay active ⁶, the exact accuracy of the device might be considered secondary. Individuals wearing activity trackers may be more health aware, thus nurses working with patients with such trackers may use it as a change agent to support the demanding process of behavioural change. ^{5, 36}

The participants of this study were limited to healthy adults; however, their BMI and level of physical activity varied, providing quite a diverse sample. A relatively small convenience sample limits the generalizability of the results. A strength of this study was that both the devices were worn on the same hand because estimates of physical activity have been reported to differ between dominant and non-dominant hands. Both devices were placed on the non-dominant hand, which should improve the validity of the measures. ³⁷ However, it

has also been suggested that there might not be a significant difference between dominant and non-dominant hands.³⁸ Each participant used the devices for a week in normal daily life; thus, the amount of data was adequate for the analyses. We were also able to exclude the days when the wear time of the smart ring and the ActiGraph differed more than 10 minutes to minimize the effects of differences in wear or sleep time estimated by the devices.

CONCLUSION

The Oura smart ring overestimated the step count compared with the wrist-worn ActiGraph accelerometer. The Oura ring showed more accuracy in measuring sedentary time. More research is, however, needed to confirm the validity of the device, as manufacturers continuously develop more sophisticated versions. The Oura smart ring cannot be unambiguously recommended to replace the ActiGraph accelerometer in measuring step count or sedentary time; however, the accuracy of the device cannot be the only criterion when choosing a wearable device for long-term use in normal daily life. Nurses might find these results beneficial while supporting their patients to be physically active.

REFERENCES

1. WHO (2018). Physical activity. Available at: <https://www.who.int/news-room/factsheets/detail/physical-activity>
2. Dohrn IM, Welmer AK, Hagströmer M. Accelerometry-assessed physical activity and sedentary time and associations with chronic disease and hospital visits – a prospective cohort study with 15 years follow-up. *Int J Behav Nutr Phys Act.* 2019;16(1):125. Doi: <https://doi.org/10.1186/s12966-019-0878-2>
3. Cerin LE, Cain LK, Oyeyemi LA, Owen FN, Conway FT, Cochrane FT, Van Dyck FD, Schipperijn FJ, Mitáš FJ, Toftager FM, Aguinaga-Ontoso FI, Sallis FJ. Correlates of agreement between accelerometry and self-reported physical activity. *Med Sci Sports Exerc.* 2016;48(6):1075–1084. Doi: 10.1249/MSS.0000000000000870
4. Wanner M, Richard A, Martin B, Faeh D, Rohrmann S. Associations between self-reported and objectively measured physical activity, sedentary behaviour and overweight/obesity in NHANES 2003-2006. *Int J Obes.* 2017;41(1):186–193. Doi: 10.1038/ijo.2016.168
5. Edward KL, Garvey L, Rahman MA. Wearable activity trackers and health awareness: nursing implications. *Int J Nurs Sci.* 2020;7(2):179–183. Doi:10.1016/j.ijnss.2020.03.006
6. Brickwood KJ, Watson G, O'Brien J, Williams AD. Consumer-based wearable activity trackers increase physical activity participation: systematic review and meta-analysis. *JMIR MHealth UHealth.* 2019;7(4):e11819. Doi: 10.2196/11819
7. Goode AP, Hall KS, Batch BC, Huffman KM, Hastings SN, Allen KD, Shaw RJ, Kanach FA, McDuffie JR, Kosinski AS, Williams JW, Gierisch JM. The impact of interventions that integrate accelerometers on physical activity and weight loss: a

- systematic review. *Ann Behav Med.* 2017;51(1):79–93. Doi: 10.1007/s12160-016-9829-1
8. Shin G, Jarrahi MH, Fei Y, Karami A, Gafinowitz N, Byun A, Lu X. Wearable activity trackers, accuracy, adoption, acceptance and health impact: a systematic literature review. *J Biomed Inform.* 2019;93:103153. Doi: 10.1016/j.jbi.2019.103153
 9. Maher C, Ryan J, Ambrosi C, Edney S. Users' experiences of wearable activity trackers: a cross-sectional study. *BMC Public Health.* 2017;17(1):880. Doi: 10.1186/s12889-017-4888-1
 10. Grym K, Niela-Vilén H, Ekholm E, Hamari L, Azimi I, Rahmani AM, Liljeberg P, Löyttyniemi E, Axelin A. Feasibility of smart wristbands for continuous monitoring during pregnancy and one month after birth. *BMC Pregnancy Childbirth.* 2019;19(1):34. Doi: 10.1186/s12884-019-2187-9
 11. Wright SP, Hall Brown TS, Collier SR, Sandberg K. How consumer physical activity monitors could transform human physiology research. *Am J Physiol Regul Integr Comp Physiol.* 2017;312(3):R358-R367. Doi: 10.1152/ajpregu.00349.2016
 12. Henriksen A, Mikalsen MH, Woldaregay AZ, Muzny M, Hartvigsen G, Hopstock LA, Grimsgaard S. Using fitness trackers and smartwatches to measure physical activity in research: analysis of consumer wrist-worn wearables. *J Med Internet Res.* 2018;20(3):e110. Doi: 10.2196/jmir.9157
 13. An HS, Jones GC, Kang SK, Welk GJ, Lee JM. How valid are wearable physical activity trackers for measuring steps? *Eur J Sport Sci.* 2017;17(3):360–368. Doi: 10.1080/17461391.2016.1255261
 14. de Zambotti M, Rosas L, Colrain IM, Baker FC. The sleep of the ring: comparison of the OURA sleep tracker against polysomnography. *Behav Sleep Med.* 2019;17(2):124–136. Doi: 10.1080/15402002.2017.1300587

15. Roberts DM, Schade MM, Mathew GM, Gartenberg D, Buxton OM. Detecting sleep using heart rate and motion data from multisensory consumer-grade wearables, relative to wrist actigraphy and polysomnography. *Sleep*. 2020;43(7):zsaa045. Doi: 10.1093/sleep/zsaa045
16. Chee NIYN, Ghorbani S, Golkashani HA, Leong RLF, Ong JL, Chee MWL. Multi-night validation of a sleep tracking ring in adolescents compared with a research Actigraph and polysomnography. *Nat Sci Sleep*. 2021;13:177–190. Doi: 10.2147/NSS.S286070
17. Asgari Mehrabadi M, Azimi I, Sarhaddi F, Axelin A, Niela-Vilen H, Myllyntausta S, Stenholm S, Dutt N, Liljeberg P, Rahmani AM. Sleep tracking of a commercially available smart ring and smartwatch against medical-grade actigraphy in everyday settings: instrument validation study. *JMIR MHealth UHealth*. 2020;8(10):e20465. Doi: 10.2196/20465.
18. Stone JD, Rentz LE, Forsey J, Ramadan J, Markwald RR, Finomore VS, Galster SM, Rezai A, Hagen JA. Evaluations of commercial sleep technologies for objective monitoring during routine sleeping conditions. *Nat Sci Sleep*. 2020;12:821–842. Doi: 10.2147/NSS.S270705
19. Chaudhry FF, Danieletto M, Golden E, Scelza J, Botwin G, Shervey M, De Freitas JK, Paranjpe I, Nadkarni GN, Miotto R, Glowe P, Stock G, Percha B, Zimmerman N, Dudley JT, Glicksberg BS. Sleep in the natural environment: a pilot study. *Sensors*. 2020;20(5):1378. doi: 10.3390/s20051378
20. Kinnunen HO, Rantanen A, Kenttä TV, Koskimäki H. Feasible assessment of recovery and cardiovascular health: accuracy of nocturnal HR and HRV assessed via ring PPG in comparison to medical grade ECG. *Physiol Meas*. 2020;41(4):04NT01. Doi: 10.1088/1361-6579/ab840a.

21. Maijala A, Kinnunen H, Koskimäki H, Jämsä T, Kangas M. Nocturnal finger skin temperature in menstrual cycle tracking: ambulatory pilot study using a wearable Oura ring. *BMC Womens Health*. 2019;19(1):150. Doi: 10.1186/s12905-019-0844-9
22. Poongodi M, Hamdi M, Malviya M, Sharma A, Dhiman G, Vimal S. Diagnosis and combating COVID-19 using wearable Oura smart ring with deep learning methods. *Pers Ubiquitous Comput*. 2021;Feb 26:1-11. Doi: 10.1007/s00779-021-01541-4.
[Online ahead of print.]
23. Moshe I, Terhorst Y, Asare KO, Sander LB, Ferreira D, Baumeister H, Mohr DC, Pulkki-Råback L. Predicting symptoms of depression and anxiety using smartphone and wearable data. *Front Psychiatry*. 2021;12:625247. Doi: 10.3389/fpsy.2021.625247
24. Henriksen A, Svartdal F, Grimsgaard S, Hartvigsen G, Hopstock L. Polar Vantage and Oura physical activity and sleep trackers: A validation and comparison study. *medRxiv preprint*. 2021. Doi: <https://doi.org/10.1101/2020.04.07.20055756>
25. Toth LP, Park S, Springer CM, Feyerabend, MD, Steeves JA, Bassett DR. Video-Recorded Validation of Wearable Step Counters under Free-living Conditions. *Med Sci Sports Exerc*. 2018;50(6), 1315–1322. Doi: 10.1249/MSS.0000000000001569
26. Pulakka A, Shiroma EJ, Harris TB, Pentti J, Vahtera J, Stenholm S. Classification and processing of 24-hour wrist accelerometer data. *J Meas Physical Behav*. 2018;1(2):51–59. Doi:10.1123/jmpb.2017-0008
27. Choi L, Capen Ward S, Schnelle JF, Buchowski MS. Assessment of wear/nonwear time classification algorithms for triaxial accelerometer. *Med Sci Sports Exerc*. 2012;44(10):2009–2016. Doi:10.1249/MSS.0b013e318258cb36
28. Koster A, Shiroma EJ, Caserotti P, Matthews CE, Chen KY, Glynn NW, Harris TB. (2016). Comparison of sedentary estimates between activPAL and Hip- and wrist-

worn ActiGraph. *Med Sci Sports Exerc.* 2016;48(8):1514–1522.

Doi:10.1249/MSS.0000000000000924

29. Suorsa K, Pulakka A, Leskinen T, Pentti J, Holtermann A, Heinonen OJ, Sunikka J, Vahtera J, Stenholm S. (2020). Comparison of sedentary time between thigh-worn and wrist-worn accelerometers. *J Meas Physical Behav.* 2020;3:234–243. Doi: <https://doi.org/10.1123/jmpb.2019-0052>
30. Cao R, Azimi I, Sarhaddi F, Niela-Vilen H, Axelin A, Liljeberg P, Rahmani AM. Accuracy Assessment of Oura Ring Nocturnal Heart Rate and Heart Rate Variability in Comparison to Electrocardiography: A Comprehensive Analysis in Time and Frequency Domains. *JMIR* 08/11/2021:27487 (forthcoming/in press)
Doi:10.2196/27487
31. Vandelanotte C, Duncan MJ, Maher CA, Schoeppe S, Rebar AL, Power DA, Short CE, Doran CM, Hayman MJ, Alley SJ. The effectiveness of a web-based computer-tailored physical activity intervention using Fitbit activity trackers: randomized trial. *J Med Internet Res.* 2018;20(12):e11321. Doi: 10.2196/11321
32. Breteler MJ, Janssen JH, Spiering W, Kalkman CJ, van Solinge WW, Dohmen DA. Measuring free-living physical activity with three commercially available activity monitors for telemonitoring purposes: validation study. *JMIR Form Res.* 2019;3(2):e11489. Doi: 10.2196/11489.
33. Degroote L, Hamerlinck G, Poels K, Maher C, Crombez G, de Bourdeaudhuih I, Vandendriessche A, Curtis RG, DeSmet A. Low-cost consumer-based trackers to measure physical activity and sleep duration among adults in free-living conditions: validation study. *JMIR MHealth UHealth.* 2020;8(5):e16674. Doi: 10.2196/16674

34. Ainsworth B, Cahalin L, Buman M, Ross R. The current state of physical activity assessment tools. *Prog Cardiovasc Dis.* 2015;57(4), 387–395. Doi: 10.1016/j.pcad.2014.10.005
35. Richards EA, Cai Y. Integrative review of nurse-delivered physical activity interventions in primary care. *West J Nurs Res.* 2016;38(4):484–507. Doi: 10.1177/0193945915581861
36. Saarikko J, Niela-Vilen H, Rahmani AM, Axelin A. Identifying target behaviors for weight management interventions for women who are overweight during pregnancy and the postpartum period: a qualitative study informed by the Behaviour Change Wheel. *BMC Pregnancy Childbirth.* 2021;21(1), 200 Doi: 10.1186/s12884-021-03689-6
37. Gjoreski M, Gjoreski H, Luštrek M, Gams M. How accurately can your wrist device recognize daily activities and detect falls? *Sensors.* 2016;16(6):800. Doi: 10.3390/s16060800
38. Dieu O, Mikulovic J, Fardy PS, Bui-Xuan G, Béghin L, Vanhelst J. Physical activity using wrist-worn accelerometers: comparison of dominant and non-dominant wrist. *Clin Physiol Funct Imaging.* 2017;37(5), 525–529. Doi: 10.1111/cpf.12337

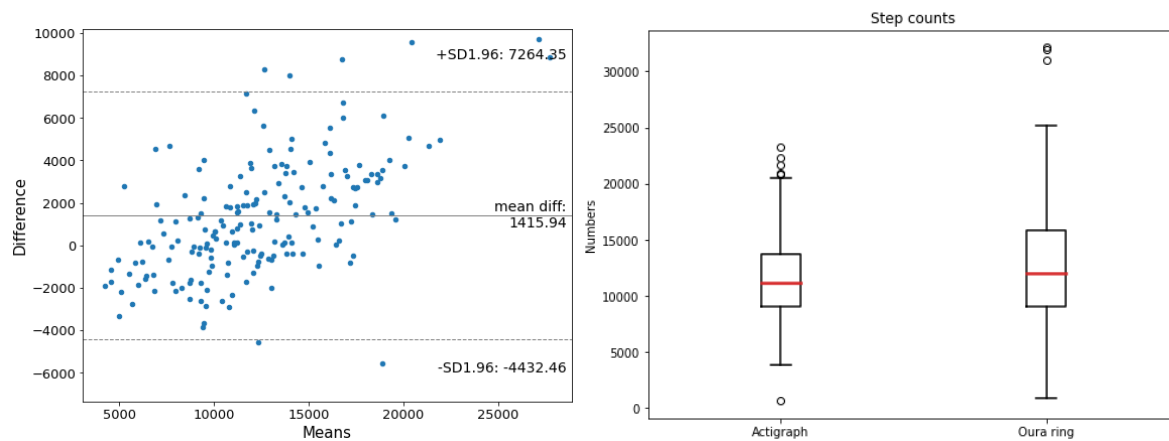


Figure 1. Bland-Altman plots and the box-plot figure of daily step counts measured by the Ora smart ring and ActiGraph accelerometer.

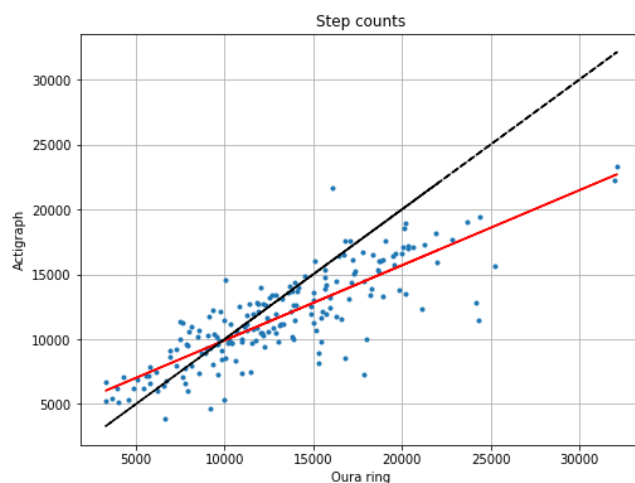


Figure 2. The scatter plots and regression analysis of daily step counts collected with the ActiGraph and the Ora ring. The regression and ideal lines (i.e., $x = y$) are shown in red and black, respectively.

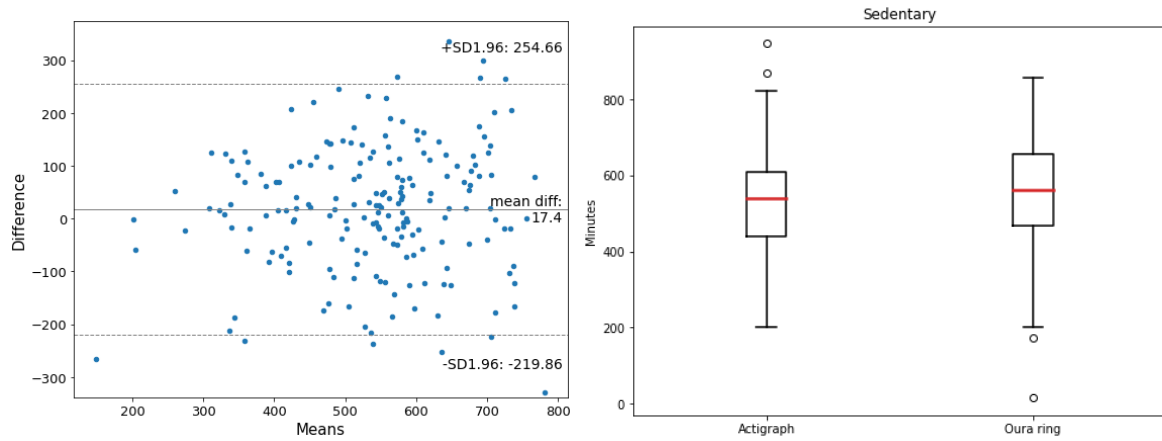


Figure 3. Bland-Altman plots and the box-plot figure of daily sedentary time measured by the Oura smart ring and the ActiGraph accelerometer.

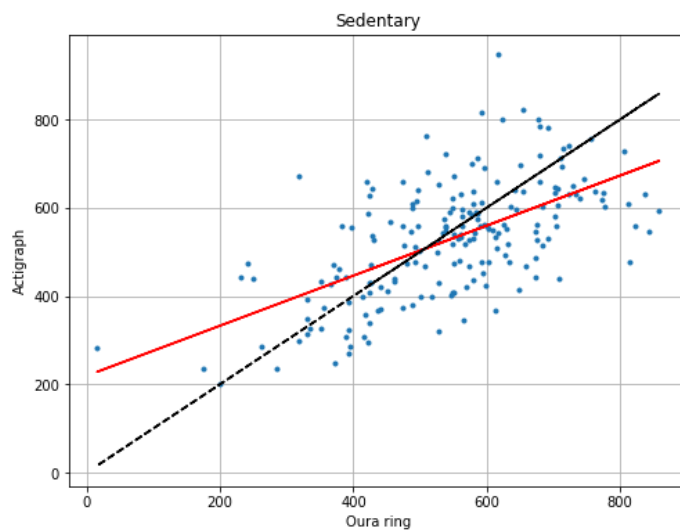


Figure 4. The scatter plots and regression analysis of daily sedentary time collected with the ActiGraph and the Oura ring. The regression and ideal lines (i.e., $x = y$) are shown in red and black, respectively.

Table 1. The characteristics of the participants (n = 42).

Variable	Median (range) / n (%)
Age, years, median (range)	32 (18–46)
BMI, kg/m ² , median (range)	24.2 (18.9–47.0)
Married/cohabiting, n (%)	33 (79)
Education level, n (%)	
<i>Elementary school</i>	1 (2.5)
<i>Secondary/vocational school</i>	9 (21)
<i>Polytechnic</i>	10 (24)
<i>University</i>	21 (50)
<i>Missing information</i>	1 (2.5)
Working status, n (%)	
<i>Employed</i>	32 (76)
<i>Unemployed</i>	1 (2.5)
<i>Student</i>	8 (19)
<i>Other</i>	1 (2.5)
Smokers, n (%)	4 (10)
Physical activity, n (%)	
<i>Daily or almost daily</i>	12 (29)
<i>Couple of times per week</i>	22 (52)
<i>Maximum of once per week</i>	8 (19)

Table 2. Mean step counts and sedentary time per day and mean difference of both variables by the Oura ring and the ActiGraph. P values are from paired t-tests.

	Step count			Sedentary time, minutes		
	Mean (95% CI)	Mean difference (95% CI)	p-value	Mean (95% CI)	Mean difference (95% CI)	p-value
Oura ring	12769 (12137, 13401)	1416 (739, 2093)	<0.001	552 (535, 568)	17 (-2, 37)	0.049
ActiGraph	11402 (10970, 11834)			528 (513, 543)		

CI = confidence interval